

Zircon M127 – A Homogeneous Reference Material for SIMS U–Pb Geochronology Combined with Hafnium, Oxygen and, Potentially, Lithium Isotope Analysis

Lutz **Nasdala** (1)*, Fernando **Corfu** (2), John W. **Valley** (3), Michael J. **Spicuzza** (3), Fu-Yuan **Wu** (4), Qiu-Li **Li** (4), Yue-Heng **Yang** (4), Chris **Fisher** (5), Carsten **Münker** (6), Allen K. **Kennedy** (7), Peter W. **Reiners** (8), Andreas **Kronz** (9), Michael **Wiedenbeck** (10), Richard **Wirth** (10), Chutimun **Chanmuang** (11,14), Manuela **Zeug** (1), Tamás **Váczi** (1,15), Nicholas **Norberg** (1,16), Tobias **Häger** (12), Alfred **Kröner** (12,13) and Wolfgang **Hofmeister** (12)

(1) Institut für Mineralogie und Kristallographie, Universität Wien, 1090 A, Wien, Austria

(2) Department of Geosciences, University of Oslo, N-0316, Oslo, Norway

(3) Department of Geoscience, University of Wisconsin, Madison, WI, 53706, USA

(4) Institute of Geology and Geophysics, Chinese Academy of Sciences, Beijing, 100029, China

(5) School of the Environment, Washington State University, Pullman, WA, 99164, USA

(6) Institut für Geologie und Mineralogie, Universität zu Köln, D-50939, Köln, Germany

(7) Department of Imaging and Applied Physics, Curtin University of Technology, Bentley, 6102, Australia

(8) Department of Geosciences, University of Arizona, Tucson, AZ, 85721, USA

(9) Geowissenschaftliches Zentrum, Georg-August-Universität Göttingen, D-37077, Göttingen, Germany

(10) Helmholtz-Zentrum Potsdam, Deutsches GeoForschungsZentrum, D-14473, Potsdam, Germany

(11) Faculty of Gems, Burapha University, Chanthaburi, 22170, Thailand

(12) Institut für Geowissenschaften, Johannes Gutenberg-Universität, D-55099, Mainz, Germany

(13) Beijing SHRIMP Center, Chinese Academy of Geological Sciences, Beijing, 100037, China

(14) Present address: Institut für Mineralogie und Kristallographie, Universität Wien, 1090 A, Wien, Austria

(15) Present address: Department of Mineralogy, Eötvös Loránd University, 1117, Budapest, Hungary

(16) Present address: PANalytical B.V., 7600AA, Almelo, The Netherlands

* Corresponding author. e-mail: lutz.nasdala@univie.ac.at

In this article, we document a detailed analytical characterisation of zircon M127, a homogeneous 12.7 carat gemstone from Ratnapura, Sri Lanka. Zircon M127 has TIMS-determined mean U–Pb radiogenic isotopic ratios of 0.084743 ± 0.000027 for $^{206}\text{Pb}/^{238}\text{U}$ and 0.67676 ± 0.00023 for $^{207}\text{Pb}/^{235}\text{U}$ (weighted means, 2s uncertainties). Its $^{206}\text{Pb}/^{238}\text{U}$ age of 524.36 ± 0.16 Ma (95% confidence uncertainty) is concordant within the uncertainties of decay constants. The $\delta^{18}\text{O}$ value (determined by laser fluorination) is $8.26 \pm 0.06\text{‰}$ VSMOW (2s), and the mean $^{176}\text{Hf}/^{177}\text{Hf}$ ratio (determined by solution ICP-MS) is 0.282396 ± 0.000004 (2s). The SIMS-determined $\delta^7\text{Li}$ value is $-0.6 \pm 0.9\text{‰}$ (2s), with a mean mass fraction of $1.0 \pm 0.1 \mu\text{g g}^{-1}$ Li (2s). Zircon M127 contains $\sim 923 \mu\text{g g}^{-1}$ U. The moderate degree of radiation damage corresponds well with the time-integrated self-irradiation dose of 1.82×10^{18} alpha events per gram. This observation, and the (U–Th)/He age of 426 ± 7 Ma (2s), which is typical of unheated Sri Lankan zircon, enable us to exclude any thermal treatment. Zircon M127 is proposed as a reference material

Dans cet article, nous documentons une caractérisation analytique détaillée du zircon M127 – une pierre précieuse homogène de 12,7 carats provenant de Ratnapura (Sri Lanka). Les rapports isotopiques radiogéniques moyens U–Pb dans Zircon M127 déterminés par TIMS sont de $0,084743 \pm 0,000027$ pour $^{206}\text{Pb}/^{238}\text{U}$ et $0,67676 \pm 0,00023$ pour $^{207}\text{Pb}/^{235}\text{U}$ (moyennes pondérées, 2s d'incertitude). L'âge $^{206}\text{Pb}/^{238}\text{U}$ obtenu de $524,36 \pm 0,16$ Ma (avec un niveau de confiance de 95%) est concordant dans la limite des incertitudes des constantes de désintégration. La valeur $\delta^{18}\text{O}$ (déterminée par fluorination laser) est de $8,26 \pm 0,06 \text{‰}$ VSMOW (2s), et le rapport moyen $^{176}\text{Hf}/^{177}\text{Hf}$ (déterminé en solution par ICP-MS) est de $0,282396 \pm 0,000004$ (2s). La valeur $\delta^7\text{Li}$ déterminée par SIMS est de $-0,6 \pm 0,9 \text{‰}$ (2s), avec une fraction de masse moyenne de $1,0 \pm 0,1 \mu\text{g g}^{-1}$ Li (2s). Le zircon M127 contient $\sim 923 \mu\text{g g}^{-1}$ U. Le degré modéré de dégâts dus à l'irradiation correspond bien à la dose intégrée dans le temps d'auto-irradiation de $1,82 \times 10^{18}$ d'événements alpha par gramme. Cette observation, et

for the determination of zircon U–Pb ages by means of SIMS in combination with hafnium and stable isotope (oxygen and potentially also lithium) determination.

Keywords: zircon, reference material, SIMS, U–Pb geochronology, oxygen isotopes, hafnium isotopes, lithium isotopes.

Received 21 Dec 15 – Accepted 06 May 16

l'âge (U-Th)/He de 426 ± 7 Ma (2s), ce qui est typique d'un zircon du Sri Lanka non chauffé, nous permettent d'exclure tout traitement thermique. Zircon M127 est proposé comme matériau de référence pour la détermination des âges U–Pb de zircon par SIMS en combinaison avec des analyses sur l'hafnium et des isotopes stables (l'oxygène et éventuellement aussi le lithium).

Mots-clés : Zircon, matériau de référence, SIMS, géochronologie U–Pb, isotopes d'oxygène, isotopes du hafnium, isotopes du lithium.

The development of the SIMS (secondary ion mass spectrometry) technique made possible the determination of U–Pb ages from polished zircon surfaces with high spatial resolution (e.g., Andersen and Hinthorne 1972, Compston *et al.* 1984, Williams 1998). SIMS is a comparative method, and the determination of accurate isotopic ratios in zircon requires calibration of the unknown results against the results of a well-characterised calibration material measured under identical conditions during the same measurement session. In principle, either a natural or synthetic reference material can be used as such a calibrant; unfortunately, well-performing synthetic reference materials for the U–Pb analysis of zircon are not available. This is due to two main reasons. First, no synthesis technique is currently available that allows one to produce homogeneous Pb-bearing zircon crystals, owing to the exceptionally low partition coefficient of Pb in zircon. Second, glass reference materials cannot be used due to their different sputtering behaviour under the oxygen ion beam, compared with that of the zircon crystals to be analysed. Consequently, high-quality natural zircon reference materials must be used and are therefore increasingly sought.

Any potentially suitable reference zircon needs to be characterised thoroughly to provide users with the best currently obtainable values, with regard to precision and accuracy, for the isotope ratios and mass fractions of the calibrant material. Also, a well-performing reference zircon needs to be exceptionally homogeneous (Pidgeon 1997, Kennedy 2000), because each individual chip, and micro-areas within chips, of the reference material must have the chemical, physical and isotopic properties of the entire, previously characterised, bulk material. Another important characteristic that determines the quality of a reference material is its reliability during analysis. In U–Pb geochronology, higher count rates – in particular for the radiogenic Pb isotope, which is always lower in abundance than the parent U isotope – lead to better Poisson statistics. This may allow the operator to shorten the analysis time and/or to decrease

the spot diameter without loss of precision. A suitable SIMS U–Pb reference should therefore contain sufficiently high concentrations of U and radiogenic Pb (whereas the concentration of non-radiogenic Pb should be negligible). However, higher levels of radiogenic Pb correlate with elevated radiation damage and this leads to an analytical difficulty, as the secondary ion sputtering behaviour under the ion beam may be different for the unknowns and reference if the structural states are sufficiently different. In searching for suitable U–Pb zircon references, it is therefore advantageous to find gem-quality specimens that have some, but not too much radiation damage. Zircon M127 fulfils all of these important prerequisites. Zircon M127 contains notably higher levels of U and radiogenic Pb isotopes than most other SIMS references, resulting in a somewhat higher level of radiation damage. The degree of damage is, however, similar to that of zircon M257, whose damage still does not cause any identifiable matrix effects under the ion beam, which might bias the SIMS results (Nasdala *et al.* 2008).

The characterisation of zircon M127 began in 2006–2008, as this specimen was among a batch of fifteen gemstones that were checked for their potential suitability as future SIMS references. After this early round of analyses, zircon M257 was preferentially selected as the first zircon to be characterised as a SIMS U–Pb reference because of its particularly large size (Nasdala *et al.* 2008), whereas zircon M127, in spite of its excellent characteristics, was not fully characterised because it was much smaller than M257. Although small amounts of M127 were used in several research projects (e.g., Mattinson *et al.* 2007, Váczi *et al.* 2009, Mattinson 2010, Guenther *et al.* 2013, Lenz and Nasdala 2015), a major fraction is still available. It has subsequently been discovered that M127 is exceptionally useful for SIMS U–Pb geochronology, especially for studies that combine U–Pb with Hf and stable isotope determination [i.e., SIMS O isotope and/or LA-ICP-MS (laser ablation-

inductively coupled plasma-mass spectrometry) using the same sample mounts. In this contribution, we therefore summarise both early and recent measurement results characterising zircon M127.

General characterisation of zircon M127

General description and preparation

Zircon M127 was a brownish oval shaped gem (Figure 1a). The cut and faceted stone weighed 2.54 g (12.7 carats), and its longest dimension was 14.5 mm. The specimen came from the collection of the Institut für Edelsteinforschung Idar-Oberstein, Germany. It was originally found in a secondary placer deposit in the Ratnapura area, which belongs to the Highland Complex, Sri Lanka (Munasinghe and Dissanayake 1981, Kröner *et al.* 1994, Zoysa 2014).

Prior to preparation, thorough homogeneity checks of the original gemstone specimen were done by (a) inspection in white-light illumination under a high-resolution optical

microscope and in an optical CL (cathodoluminescence) microscope, and by (b) multiple laser spectroscopy analyses placed on different faces and under different sample orientations. The stone was found to be internally flawless, free of noticeable fractures and uniform in colour. Neither inclusions nor growth zoning or other heterogeneities were observed. The initial Raman and laser-induced PL (photoluminescence) analyses indicated that zircon M127 has a uniform, moderate degree of radiation damage (Figure 2a) and uniform rare earth element (REE) emission patterns (Figure 2b).

The stone was cut in half along its longest dimension, and halves were cut into ~2.5-mm-thick slices (Figure 1b), using a 200- μm , diamond-trimmed tungsten wire. Slices were then crushed in a steel cylinder apparatus. The central slice pictured in Figure 1b (maximum dimension ~8 mm) was cut again very close to one of the large side planes, that is parallel to the initial cut direction. This was performed to produce one particularly large, doubly polished thin section for homogeneity tests.

Chemical composition and homogeneity

Contents of major elements were measured by means of electron probe micro-analysis (EPMA). Multiple spots ($n = 63$) were measured across two large slices of M127, including the ~8-mm-thin section. These wavelength-dispersive X-ray analyses were performed using the Jeol 8900 RL EPMA system at Geowissenschaftliches Zentrum, Universität Göttingen, Germany. The accelerating voltage was 20 kV, and the beam current was set at 80 nA. The electron beam was focussed to a spot area 2 μm in diameter. Analyses of zircon M127 were performed in the same session as those of zircon M257; hence, experimental details correspond to the detailed description in Nasdala *et al.* (2008). Counting times varied between 15 s peak and 2×5 s backgrounds for main elements (Zr–K $_{\alpha}$, Si–K $_{\alpha}$) up to 300 s peak and 2×150 s backgrounds for actinides (U–M $_{\alpha}$ and Th–M $_{\alpha}$). Synthetic calibrant materials were used, including ZrSiO $_4$ (for Zr and Si), HfSiO $_4$ (for Hf), YAG (yttrium aluminium garnet, for Y), Yb-glass (for Yb), apatite (for P), wollastonite (for Ca), Al $_2$ O $_3$ (for Al), haematite (for Fe), ThSiO $_4$ (for Th) and UO $_2$ (for U). Data were processed using the CITZAF routine in the JEOL software, which is based on the $\phi(\rho z)$ method (Armstrong 1991, 1995).

Prior to EPMA analysis, detailed imaging was performed using the large, 8-mm-thin section as well as seven smaller chips embedded in epoxy sample mounts and polished. First, slices and chips were inspected under a research-grade optical microscope. Neither inclusion nor growth or




Figure 1. White-light photographs of zircon M127, a clear, dark brownish, cut and faceted gemstone originating from Ratnapura, Sri Lanka. (a) Original stone as purchased. (b) One half after cutting into five slices. [Colour figure can be viewed at wileyonlinelibrary.com].




Figure 2. Spectroscopy of zircon M127. (a) Raman spectra in the SiO₄ stretching range, showing M127 in comparison with three zircon reference materials ranging from very well crystallised (Penglai; spectrum this work; for sample description, see Li *et al.* 2010), mildly radiation damaged (91 500, data from Wiedenbeck *et al.* 2004) to strongly radiation damaged (OR1, data from Nasdala *et al.* 2004). (b) The PL spectrum (473 nm excitation) of M127 is dominated by groups of narrow, REE-related emissions (For assignment, see Gaft *et al.* (2000) and Lenz and Nasdala (2015)).

other zoning was found; uniform interference colours were observed in cross-polarised light. Second, back-scattered electron (BSE) and panchromatic CL imaging were performed using the EPMA. All BSE and CL images revealed uniform grey scale intensity, and neither primary growth zoning nor other internal heterogeneities were observed. In view of the particularly high sensitivity of the CL technique to reveal internal textures (for a summary see Corfu *et al.* 2003), the apparent absence of any heterogeneity in all CL images obtained supports the internal homogeneity of zircon M127.

Trace element analysis of zircon M127 by means of LA-ICP-MS was performed in 2006 by Jan Košler (deceased), University of Bergen, Norway, as part of the characterisation of zircon M257. Analyses were performed using a ThermoFinnigan Element2 single-collector double-focussing magnetic-sector system coupled to a NewWave/Merchandek UP213 laser. Analytical details and data reduction are described elsewhere (Nasdala *et al.* 2008). In addition, a fairly large amount of M127 (~ 300 mg) was subjected to a solution ICP-MS analysis at GEUS (Nationale Geologiske Undersøgelser for Danmark og Grønland), Copenhagen, Denmark. This was performed in 2008, to determine reliably the U mass fraction of M127. Zircon M127 was then used to

recalibrate the U data obtained by EPMA for zircon M257 (for discussion and analytical details see Nasdala *et al.* 2008).

The EPMA and LA-ICP-MS results are presented in Table 1. Zircon M127 contains rather moderate levels of non-formula elements; only the hafnium-oxide content (1.50% *m/m*) is in the per cent range. The uranium mass fraction was determined by solution ICP-MS at ~ 923 μg g⁻¹ U (Nasdala *et al.* 2008). This value is considerably higher than in most other zircon reference materials [with the exception of M257 whose U mass fraction (~ 840 μg g⁻¹) is at a similar level]. The Th/U weight ratio of zircon M127 is ~ 0.45. This ratio is not unusual for Sri Lankan zircon (Murakami *et al.* 1991, Nasdala *et al.* 2004); however, it should be noted that the value of ~ 0.45 is much higher than 1/9, which was postulated as typical 'Sri Lankan' actinide concentration ratio by Holland and Gottfried (1955). The homogeneity of the chemical composition, and in particular of the U and Th mass fractions, was checked by two line scans across a large polished chip of zircon M127. Results obtained along a ~ 7.8-mm-long traverse are plotted in Figure 3. No lateral chemical variations exceeding the measurement uncertainties were found.

Table 1.
Chemical composition of zircon M127 (EPMA, University of Göttingen; LA-ICP-MS, University of Bergen)

EPMA results (n = 63) ^a		LA-ICP-MS results (n = 24)					
Oxide	Mass fraction (% m/m) ^b	Element	Isotope measured	Mass fraction (µg g ⁻¹) ^b	Element	Isotope measured	Mass fraction (µg g ⁻¹) ^b
SiO ₂	32.6 ± 0.2	Y	89	785 ± 55	Dy	163	67.1 ± 2.0
P ₂ O ₅	0.057 ± 0.006	Nb	93	1.61 ± 0.45	Ho	165	25.7 ± 1.6
Y ₂ O ₃	0.109 ± 0.012	La	139	0.35 ± 0.17	Er	166	121 ± 9
ZrO ₂	65.9 ± 0.3	Ce	140	16.9 ± 0.8	Tm	169	28.0 ± 2.1
Yb ₂ O ₃	0.028 ± 0.012	Pr	141	0.18 ± 0.07	Yb	172	286 ± 19
HfO ₂	1.50 ± 0.02	Nd	146	1.95 ± 0.56	Lu	175	53.7 ± 1.8
ThO ₂	0.046 ± 0.006	Sm	147	3.95 ± 0.65	Hf	178	12400 ± 500
UO ₂	0.099 ± 0.008	Eu	153	0.39 ± 0.13	Pb	206	78.4 ± 4.2
Total	100.4 ± 0.4	Gd	157	15.6 ± 1.5	Th	232	413 ± 17
		Tb	159	5.55 ± 0.36	U	238	896 ± 36 ^c

^a Al₂O₃, CaO and FeO were not detected or averages were below 0.005% m/m.

^b Quoted uncertainties are 2s.

^c The U mass fraction was determined by solution ICP-MS at ~ 923 µg g⁻¹ (Nasdala *et al.* 2008), which is suggested to be used as the 'working value'.

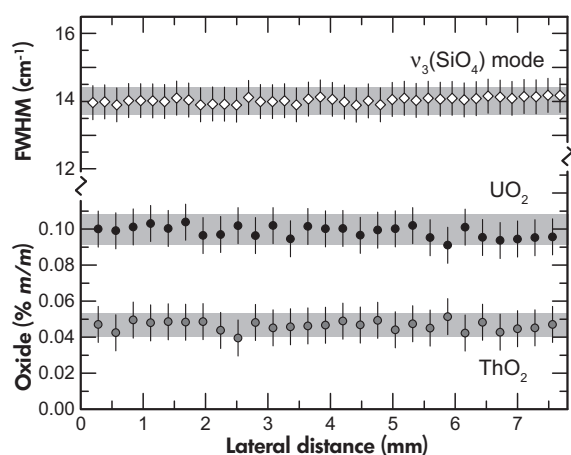


Figure 3. Results of Raman microprobe and EPMA line scans across an ~8-mm-long traverse. Lateral variations of observed Raman and concentration parameters were below the measurement uncertainties (visualised by grey bars).

The REE mass fractions found (Table 1) are typical of igneous zircon (Figure 4; compare Hoskin and Schaltegger 2003). Also, the REE pattern is typical of unaltered zircon from igneous crustal rocks (Hoskin and Schaltegger 2003). First, the HREEs (heavy rare earth elements) are enriched relative to the middle and light REE (Figure 4). Second, a positive Ce anomaly (Ce/Ce* = 1.54) and a negative europium anomaly (Eu/Eu* = 0.13) were observed. The former (i.e., HREE enrichment) was also evident in the PL spectrum (Figure 2b) where strong emissions were observed for the trivalent Dy and Tm, and to a lesser extent Sm (Gaff *et al.* 2000, Lenz *et al.* 2015).

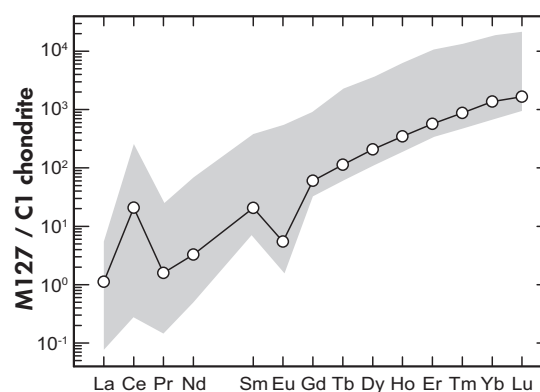


Figure 4. Plot of chondrite-normalised REE mass fractions determined by LA-ICP-MS (University of Bergen). The grey area visualises REE mass fraction ranges obtained for unaltered igneous zircon (graphically extracted from figures 4 and 5 in Hoskin and Schaltegger 2003).

Finally, it is important to note that elemental species, such as Ca, P and Fe that are typically excluded or low in primary zircon but are often absorbed extensively during alteration events (Smith *et al.* 1991, Geisler *et al.* 2003, Pérez-Soba *et al.* 2007, Nasdala *et al.* 2010), have low mass fractions in zircon M127 (Table 1). This observation shows that M127 has not undergone intense weathering or other postcrystallisation chemical alteration.

Structural state and radiation damage

Natural zircon may have appreciable structural damage created by alpha decay of U and Th and their unstable

daughter nuclei. The accumulation of this damage leads to systematic changes of physical parameters, which in turn can be used to estimate the degree of radiation damage sustained by an unknown zircon sample. We have therefore applied a number of measurement techniques for characterising the structural state of M127 (by determining specific gravity, unit-cell parameters, Raman spectral parameters and sharpness of electron diffraction maxima). This was performed to check the degree to which the observed deviation from the ideal structural state corresponds, within the well-known 'Sri Lankan trend', to the calculated self-irradiation. Obvious mismatches, in turn, could unravel structural recovery as for instance caused by postgrowth alteration or synthetic thermal gem enhancement.

The self-irradiation causing the radiation damage is quantified commonly by the alpha dose (D_α), that is the time-integrated number of alpha-decay events experienced by the zircon since primary growth (more precisely, since the time of closure of the U–Pb system). This parameter is calculated according to (Murakami *et al.* 1991, Nasdala *et al.* 2001)

$$D_\alpha = \frac{6 \cdot c_{Th} \cdot N_A}{10^6 \cdot M_{232}} \cdot (e^{\lambda_{232} t} - 1) + \frac{7 \cdot c_U \cdot 0.0072 \cdot N_A}{10^6 \cdot M_{235}} \cdot (e^{\lambda_{235} t} - 1) + \frac{8 \cdot c_U \cdot 0.9928 \cdot N_A}{10^6 \cdot M_{238}} \cdot (e^{\lambda_{238} t} - 1) \quad (1)$$

where c_U and c_{Th} = U and Th mass fractions in $\mu\text{g g}^{-1}$ (Table 1); N_A = Avogadro's number; M_{238} , M_{235} and M_{232} = molecular weights of isotopes; λ_{238} , λ_{235} and λ_{232} = decay constants of ^{238}U , ^{235}U and ^{232}Th ; and t = zircon U–Pb age (here 524.3 Ma; see below). It should be noted that the common use of the U–Pb age in calculating D_α adds slight uncertainty, as this practice is based on the – often incorrect – assumption that the closure of structural recovery by annealing corresponds exactly with U–Pb system closure. For natural zircon, D_α actually is not a 'measure' of the structural damage present in a given natural zircon sample. Rather, D_α quantifies the total self-irradiation since the time of closure of the U–Pb system. How much of the damage has been accumulated or has been thermally annealed depends on the thermal history of the sample. Nasdala *et al.* (2001, 2004) and Palenik *et al.* (2003) found that the Ratnapura, Sri Lanka, gem zircon suite is not as radiation damaged as expected given the U and Th mass fractions and ages; only about 55% of the damage was retained. This is assigned to the particular geological history of the area (involving slow cooling prior to Ordovician uplift and perhaps a reheating event; Nasdala *et al.* 2004). In summary, radiation damage cannot be compared

among samples of different origin by the simple evaluation of their calculated D_α values. However, internal comparison is straightforward with Sri Lankan zircon gems, because – provided no gem enhancement involving elevated temperatures was applied – they all show uniform trends of parameter changes depending on D_α (Nasdala *et al.* 2004). The calculated value of $D_\alpha = 1.82 \times 10^{18}$ events per gram for zircon M127 is rather moderate. It is well below the first percolation point (for Sri Lanka zircon determined at $\sim 3.5 \times 10^{18} \alpha \text{ g}^{-1}$; Salje *et al.* 1999) that is characterised by the beginning of three-dimensional interconnection of amorphous clusters in the crystalline matrix. The nearly complete transformation of Sri Lankan zircon to the amorphous state requires self-irradiation doses of $\sim 10^{19} \alpha \text{ g}^{-1}$ (Salje *et al.* 1999, Nasdala *et al.* 2002). The calculated alpha dose of 1.82×10^{18} events hence suggests a notable but still moderate level of radioactive self-irradiation.

The specific gravity of zircon M127 was determined at $4.625 \pm 0.005 \text{ g cm}^{-3}$. This was performed prior to preparation, by repeated weighing of the original stone in air and in distilled water. The gravity of M127 is $\sim 2\%$ lower than that of crystalline zircon ($> 4.7 \text{ g cm}^{-3}$) but well above than that of metamict zircon ($< 4 \text{ g cm}^{-3}$; e.g., Sahama 1981, Nasdala *et al.* 2002), indicating a notable, but still moderate degree of self-irradiation induced volume expansion. As zircon M127 has a 'regular' chemical composition with generally low amounts of non-formula elements, and as it is free of inclusions, any chemical or textural effects on the sample's specific gravity must be very minor. The moderately decreased specific gravity is therefore assigned solely to the moderate degree of radiation damage present.

Unit-cell dimensions of zircon M127 were determined from four 50- to 100- μm -sized chips, by obtaining ten frames each on a Bruker Nonius KappaCCD single-crystal X-ray diffractometer. Analyses were performed with Mo–K α radiation. The distance between chip and detector was 35 mm. The measurement time per frame (width 2°) was 3 s. The dimensions of the tetragonal unit-cell were determined at $a_0 = 6.6408(4) \text{ \AA}$ and $c_0 = 6.0367(5) \text{ \AA}$ (Figure 5), resulting in a unit-cell volume of $V = 266.22(4) \text{ \AA}^3$. Compared with well-crystallised zircon, zircon M127 is characterised by expansion of the unit cell of $\sim 2\%$. First, this corresponds very well with the $\sim 2\%$ decrease of the specific gravity (cf. above). Second, the $\sim 2\%$ cell expansion characterises the material as moderately radiation damaged (Holland and Gottfried 1955, Murakami *et al.* 1991). Note that the observed expansion of parameters a_0 and c_0 is rather 'homogeneous' (Holland and Gottfried 1955, compare also figure 6A in Nasdala *et al.* 2004). Partially

annealed zircon, in contrast, is typically characterised by an apparent a_0 - c_0 mismatch, caused by preferential recovery of the original expansion along the crystallographic a axis (Weber 1990, 1993).

The degree of radiation damage was further estimated from the full width at half-maximum (FWHM) of the main Raman band of zircon ($\nu_3(\text{SiO}_4)$ vibrational mode; Nasdala *et al.* 1995, 2001). Spectra were obtained with He-Ne 632.8 nm excitation (8 mW at the sample surface) by means of a Horiba LabRam HR Evolution system (focal length 800 mm). A diffraction grating with 1800 grooves mm^{-1} was placed in the optical pathway, resulting in a spectral resolution of $\sim 0.8 \text{ cm}^{-1}$. The system's wavenumber accuracy is better than 0.5 cm^{-1} ; wavenumber calibration was performed using the Rayleigh line and emission lines of a Kr lamp. Raman spectra were corrected for background and fitted assuming Lorentzian–Gaussian band shapes. Real FWHM values were calculated by correcting measured FWHMs for the instrumental profile function of the spectrometer (Dijkman and van der Maas 1976, Nasdala *et al.* 2001, Vácz 2014). The Raman spectrum of zircon M127 is moderately broadened but bands are still very symmetrical (Figure 2a). The FWHM of the $\nu_3(\text{SiO}_4)$ band (here observed at $999.8 \pm 0.5 \text{ cm}^{-1}$) was determined at $14.0 \pm 0.4 \text{ cm}^{-1}$ (Figure 5), which indicates significant but still moderate radiation damage. Raman line scans did not reveal lateral variations of Raman parameters (Figure 3), implying that the moderate radiation damage in zircon M127 is homogeneous.

Electron diffraction was performed by means of a FEI Tecnai G² F20 X-Twin TEM (transmission electron microscope) system at Helmholtz-Zentrum Potsdam. The TEM system was operated at 200 kV and 0.5 nA beam current. For TEM analysis, thin foils were cut out of polished mounts containing oriented zircon chips using a FEI FIB200 (for details of the focussed ion beam technique see Wirth 2004). An electron diffraction pattern of zircon M127 is shown in Figure 6a. The diffraction pattern of M127 appears somewhat ‘blurred’ when compared with that of crystalline zircon, whereas no ‘amorphous’ diffraction ring (which is typical of highly radiation-damaged zircon; Nasdala *et al.* 2004) is observed. The former observation is visualised in Figure 6b, which shows the diffraction intensity along the line marked in Figure 6a. The intensity profile was extracted using the ImageJ software (Schneider *et al.* 2012). The analogous intensity profile of a nearly undamaged zircon (sample Rata described in Lenz and Nasdala 2015) obtained with the same TEM system under identical experimental conditions shows notably narrower diffraction maxima (Figure 6b).

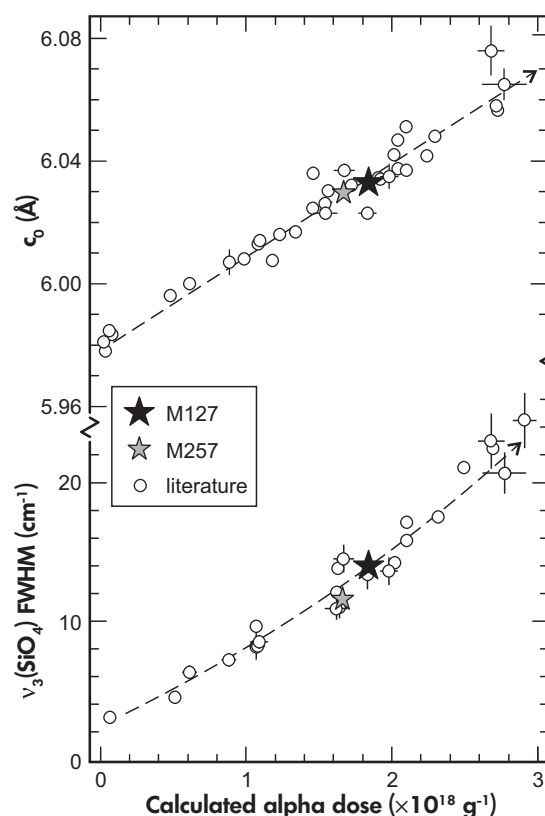


Figure 5. Plots of unit-cell parameter c_0 and the width of the main Raman band at $\sim 1000 \text{ cm}^{-1}$ against the time-integrated alpha dose, for zircon samples from Sri Lanka. Literature data for unit-cell constants from Holland (1954), Murakami *et al.* (1991) and Nasdala *et al.* (2004). Literature data for Raman FWHMs from Zhang *et al.* (2000) and Nasdala *et al.* (2001, 2004). Data for zircon M257 from Nasdala *et al.* (2008). Note that parameters of zircon M127 plot well within the ‘Sri Lankan’ trends (visualised by dashed arrows).

All of our results indicate that the structure of zircon M127 is moderately damaged due exclusively to radioactive self-irradiation over geological periods of time. This conclusion is supported by the observations that the specific gravity, the unit-cell volume and the Raman band broadening correspond well, within the ‘Sri Lankan’ trends of parameter changes, with an alpha dose of $1.82 \times 10^{18} \text{ g}^{-1}$ (Figure 5). The degree of damage is significantly higher than most other zircon references, such as Penglai (for sample description see Li *et al.* 2010), 91500 (Wiedenbeck *et al.* 2004), and CZ3 (Nasdala *et al.* 2004, for sample description see Pidgeon 1997). The degree of radiation damage in M127 is, however, still moderate, very similar to the structural disorder of zircon M257 (Norberg 2007, Nasdala *et al.* 2008). As M257 does not show any significant matrix effects (such as preferred sputtering of Pb

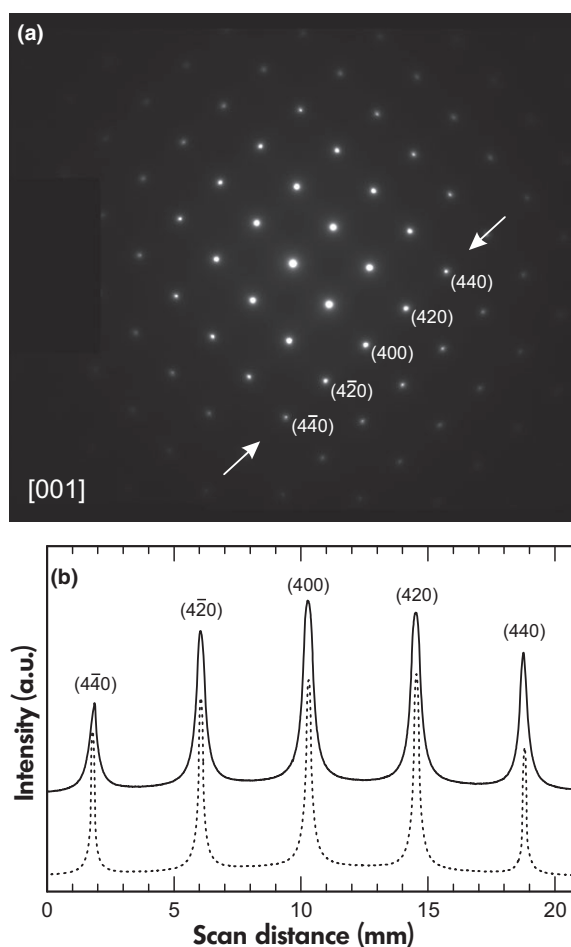


Figure 6. Electron diffraction in the TEM. (a) Photograph of the diffraction pattern of zircon M127 observed along [001]. (b) Plot of the intensity distribution along the line marked in a with arrows (solid graph), in comparison with an analogous intensity distribution pattern obtained from highly crystalline zircon from Ban Lung, Ratanakiri, Cambodia (dotted graph; for sample description, see Lenz and Nasdala 2015). Graphs are shown with vertical offset for clarity.

from highly radiation-damaged zircon; e.g., McLaren *et al.* 1994, Nasdala *et al.* 2002), such problems are also not to be expected for M127.

Isotopic composition of zircon M127

U–Pb age determination by TIMS

The U–Pb age of zircon M127 was determined by thermal ionisation mass spectrometry (TIMS) analysis in the geochronology laboratories of the University of California at Santa Barbara, USA, and University of Oslo, Norway. Results of chemical abrasion (CA) TIMS analyses of one 1.437-mg

chip at the University of California have already been published elsewhere (Mattinson 2010).

At the University of Oslo, one 0.646-mg chip of M127 was subjected to isotope dilution (ID) TIMS analysis. The chip was cleaned with HNO₃, H₂O and acetone, then weighed on a microbalance and transferred to a Krogh-type bomb (see Krogh 1973), to which a measured amount of ²⁰²Pb–²⁰⁵Pb–²³⁵U spike was added. The spike was evaporated before adding a mixture of HF and HNO₃ (12:1). The bomb was placed in an oven for 5 d at 190 °C. The solution was then evaporated to dryness and redissolved in 3 mol l⁻¹ HCl overnight at 190 °C. The solution was then split with a pipette onto four columns with anion exchange resin to separate out Pb and U. The latter were then loaded on zone-refined Re filaments together with Si gel and H₃PO₄ and measured in a MAT262 mass spectrometer. The main Pb and U peaks were measured on multiple Faraday cups in static mode, and the ²⁰⁷Pb/²⁰⁴Pb ratio was measured by peak-jumping on an electron multiplier. Other details of the procedure can be found in Corfu (2004). The spike composition was calibrated against the synthetic ET100 solution (Condon *et al.* 2008) provided by the EARTHTIME initiative (<http://www.earthtime.org>).

The ²³⁸U decay constant of Jaffey *et al.* (1971; 1.55125 × 10⁻¹⁰ a⁻¹) and the re-revised ²³⁵U decay constant of Mattinson (2010; 9.8571 × 10⁻¹⁰ a⁻¹), which is marginally higher than the revised value of Schoene *et al.* (2006; 9.8569 × 10⁻¹⁰ a⁻¹), were used for converting isotopic ratios into ages and for plotting the results. Age calculations and the preparation of the Concordia plot were performed using the Isoplot program (Ludwig 2003). Note that isotopic ratios are reported as measured (i.e., without Th fractionation correction). The uncertainties reported include quadratically propagated measurement errors, a minimum reproducibility term of ± 0.06% amu⁻¹ on the fractionation corrections for Pb and U (based on regular runs of standard solutions), blank corrections of 2 ± 1 pg Pb and 0.1 ± 0.05 pg U and uncertainties of 2% on the ²⁰⁶Pb/²⁰⁴Pb and 1% on the ²⁰⁷Pb/²⁰⁴Pb compositions of the blank.

The U–Pb results obtained in the University of Oslo laboratory are summarised in Table 2, and a Concordia plot including both these results and the results of Mattinson (2010) is presented in Figure 7. From all twenty TIMS analyses, a weighted mean ²⁰⁶Pb/²³⁸U ratio for zircon M127 of 0.084743 ± 0.000027 (2s) was calculated, which corresponds to a ²⁰⁶Pb/²³⁸U age of 524.36 ± 0.16 Ma (uncertainty quoted at the 95% confidence

Table 2.
Results of ID-TIMS U–Pb analyses of M127 (University of Oslo)

Analysis number	Pb ($\mu\text{g g}^{-1}$)	U ($\mu\text{g g}^{-1}$)	Th/U	Total common Pb (pg)	$^{207}\text{Pb}/^{235}\text{U}$	2s (abs.)	$^{207}\text{Pb}/^{235}\text{U}$ age (Ma)	$^{206}\text{Pb}/^{238}\text{U}$	2s (abs.)	$^{206}\text{Pb}/^{238}\text{U}$ age (Ma)	ρ (err. corr.)	$^{207}\text{Pb}/^{206}\text{Pb}$	2s (abs.)	Discordance (%)
153/53A	72	817	0.45	7.5	0.67763	0.00201	524.88 \pm 1.22	0.084856	0.00023	525.04 \pm 1.38	0.98	0.057917	0.00004	-0.2
153/53B	72	816	0.45	8.6	0.67689	0.00271	524.44 \pm 1.64	0.084798	0.00031	524.70 \pm 1.86	0.98	0.057894	0.00005	-0.3
153/53C	72	816	0.45	9.8	0.67838	0.00275	525.34 \pm 1.66	0.084956	0.00032	525.64 \pm 1.88	0.97	0.057914	0.00006	-0.3
153/53D	72	817	0.46	8.7	0.67785	0.00283	525.02 \pm 1.71	0.084876	0.00032	525.16 \pm 1.90	0.97	0.057923	0.00006	-0.2
ID-TIMS means:					0.67769	0.084871						0.057912		
Mean Concordia age of all four analyses: 525.01 \pm 0.92 Ma (95% conf.)														

One 646- μg chip was dissolved (split after dissolution).

level). The weighted mean $^{207}\text{Pb}/^{235}\text{U}$ isotopic ratio was calculated at 0.67676 ± 0.00023 (2s). The mean Concordia age calculated is 524.37 ± 0.46 Ma (95% confidence; errors of decay constants included). The U–Pb system of zircon M127 is well concordant within the uncertainties of the decay constants (for further discussion, see Schoene *et al.* 2006, Schmitz and Schoene 2007, Mattinson 2010). We recommend the above mean isotopic ratios and $^{206}\text{Pb}/^{238}\text{U}$ age to be used when applying zircon M127 as reference material in SIMS U–Pb dating.

Hafnium isotope determination by solution ICP-MS

Hafnium mass fractions, and $^{176}\text{Hf}/^{177}\text{Hf}$ and $^{176}\text{Lu}/^{177}\text{Hf}$ ratios, were measured by solution isotope dilution analysis. Three multi-collector ICP-MS systems at different laboratories were used: the Radiogenic Isotope and Geochronology Laboratory (RIGL) at Washington State University (WSU), Pullman; the Institute of Geology and Geophysics, Chinese Academy of Sciences (IGGCAS), Beijing; and the joint Köln-Bonn laboratory, Germany. To check for the internal homogeneity of Hf isotopes within zircon M127, each of the three laboratories was provided with five small samples (1–3 mg per sample consisting of one, two or three individual chips). The five samples were recovered from the five main slices of the original gemstone (see Figure 1b; one sample per slice).

In the RIGL facility, each fragment was separately dissolved in a mixture of concentrated HF and HNO_3 in pre-cleaned 0.5 ml Savillex[®] perfluoroalkoxy screw-top vials. The vials were loosely capped and placed in Teflon[®] liner in a large-capacity Parr dissolution bomb to which ~ 5 ml of concentrated HF was added to provide vapour pressure within the bomb. The sealed bomb was placed in an oven at 250 °C for 48 hr. Following dissolution, the contents of each bomb were transferred to a 7 ml Savillex[®] beaker, dried and fluxed overnight in a mixture of 2.5 mol l⁻¹ HCl/ H_3BO_3 to convert to chlorides and minimise production of fluoride species. Samples were again dried and redissolved in 1 ml 1 mol l⁻¹ HCl plus 0.1 mol l⁻¹ HF (precisely weighed). From this solution, an aliquot for analysis was removed and added to a clean 7 ml Savillex[®] beaker to which a zircon-specific mixed ^{176}Lu – ^{180}Hf tracer solution was added. Further details of sample preparation, column chemistry and Hf and Lu mass spectrometry are described in Vervoort *et al.* (2004) and Goodge and Vervoort (2006). The purified Hf of samples (and calibrants) were run as 50 ng ml⁻¹ solutions and introduced to the RIGL ThermoFinnigan Neptune MC-ICP-MS using an Aridus desolvating nebuliser. Mass fractionation was internally corrected using $^{179}\text{Hf}/^{177}\text{Hf} = 0.7325$, and all sample analyses were normalised using the Hf isotope reference

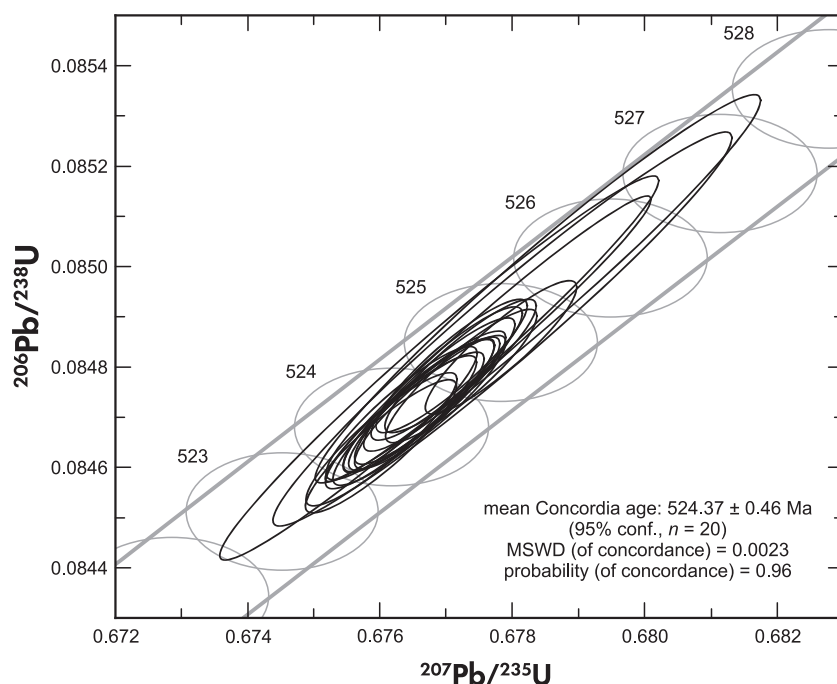


Figure 7. Concordia plot of U-Pb data obtained at the University of California at Santa Barbara (CA-TIMS; sixteen plateau steps, data from Mattinson 2010) and at the University of Oslo (ID-TIMS, four individual analyses). All ellipses represent 2s uncertainties. The uncertainty of the mean age quoted includes uncertainties of decay constants.

material JMC 475 (Patchett and Tatsumoto 1980; with a presently accepted value of $^{176}\text{Hf}/^{177}\text{Hf} = 0.282160$). Five analyses of JMC 475 were interspersed between samples and yielded a mean $^{176}\text{Hf}/^{177}\text{Hf} = 0.282132 \pm 0.000004$ (2s; $n = 5$).

For analyses at the IGGCAS, single chips of zircon M127 were weighed and dissolved in HF-HNO₃ in 3-ml vials placed in high-pressure bombs at 210 °C for 1 w. Afterwards, the samples were dried down and redissolved in 3 mol l⁻¹ HCl. Each sample solution was then split. About 20% was spiked with a mixed ¹⁷⁶Lu and ¹⁸⁰Hf tracer for determining the Lu and Hf mass fractions. The spike solution used was calibrated beforehand against a standard solution made from pure metals (Yang *et al.* 2010). It was tested on several international calibrants (BCR-2, W-2) and yielded results corresponding to reference values (Münker *et al.* 2001). The remaining ~ 80% of each initial sample solution was used to determine the Hf isotopic composition. The chemical purification procedure described in Nebel-Jacobsen *et al.* (2005) and Morel *et al.* (2008) was applied. Isotope measurements were performed on a Thermo Scientific Fisher Neptune MC-ICP-MS following the protocol listed in Yang *et al.* (2010). Instrumental mass bias was corrected offline using the exponential law and $^{179}\text{Hf}/^{177}\text{Hf} = 0.7325$. For possible interferences of ¹⁷⁶Yb and ¹⁷⁶Lu on ¹⁷⁶Hf,

isotopes ¹⁷³Yb and ¹⁷⁵Lu were monitored and corrected for, applying $^{176}\text{Lu}/^{175}\text{Lu} = 0.02655$ and $^{176}\text{Yb}/^{173}\text{Yb} = 0.79631$ (Vervoort *et al.* 2004). The $^{176}\text{Hf}/^{177}\text{Hf}$ results for M127 are reported relative to a value of 0.282160 for JMC 475.

The procedure in the Köln-Bonn laboratory was broadly similar. Lutetium and Hf isotope measurements were performed using a Thermo Neptune MC-ICP-MS and a procedure after Nebel-Jacobsen *et al.* (2005), employing a mixed ¹⁷⁶Lu-¹⁸⁰Hf tracer specifically designed for zircon. Results for $^{176}\text{Hf}/^{177}\text{Hf}$ are given relative to a value of 0.282160 for the Münster AMEs standard solution that is isotopically indistinguishable from JMC 475.

All results are presented in Table 3 and Figure 8. They indicate that zircon M127 is fairly uniform in Hf mass fraction and $^{176}\text{Hf}/^{177}\text{Hf}$ ratio. Considering all eighteen individual analyses (but without consideration of re-analyses which are merely reported for completeness), the unweighted mean $^{176}\text{Hf}/^{177}\text{Hf}$ ratio is determined at 0.282396 ± 0.000004 (2s), which we suggest be used as a 'working value'. The $^{176}\text{Hf}/^{177}\text{Hf}$ ratios determined in Köln may seem to be slightly higher compared with data produced in the two other laboratories. Differences among the three laboratories are, however, within measurement uncertainties and hence cannot be considered systematic.

Table 3.
Results of Hf isotope determinations by solution ICP-MS

Laboratory	Analysis number	Lu ($\mu\text{g g}^{-1}$)	Hf ($\mu\text{g g}^{-1}$)	$^{176}\text{Lu}/^{177}\text{Hf}$	$^{176}\text{Hf}/^{177}\text{Hf}^{\text{a}}$	2s (abs.)	$^{176}\text{Hf}/^{177}\text{Hf}^{\text{b}}$
Academy of Sciences, Beijing	M127 #1A	46.7	12497	0.00053	0.282393	0.000006	0.282388
	M127 #1A re-analysis				0.282385	0.000007	
	M127 #2D	78.0	12441	0.00089	0.282392	0.000006	0.282383
	M127 #2D re-analysis				0.282385	0.000005	
	M127 #3D	67.9	12239	0.00079	0.282396	0.000004	0.282388
	M127 #3D re-analysis				0.282392	0.000005	
	M127 #4B	81.1	11493	0.00100	0.282388	0.000006	0.282378
	M127 #4B re-analysis				0.282388	0.000006	
	M127 #5B	60.8	12227	0.00071	0.282390	0.000009	0.282383
	M127 #5B re-analysis				0.282400	0.000008	
	M127 #6Y	51.6	12301	0.00060	0.282391	0.000006	0.282385
	M127 #6Y re-analysis				0.282388	0.000007	
Mean observed $^{176}\text{Hf}/^{177}\text{Hf}$ ratio of six ^c analyses: 0.282392 ± 0.000006 (2s)							
Washington State University, Pullman	11-chip 3	64.5	12616	0.00073	0.282397	0.000006	0.282390
	11-chip 3 re-analysis				0.282402	0.000006	
	Chip 12	103.1	12590	0.00116	0.282401	0.000009	0.282389
	Chip 12 re-analysis				0.282395	0.000006	
	Chip 13	48.8	12529	0.00055	0.282394	0.000008	0.282389
	14-chip 1	78.7	12578	0.00089	0.282395	0.000008	0.282386
	14-chip 2	68.7	12604	0.00077	0.282388	0.000006	0.282380
	15-chip 1	69.6	12539	0.00079	0.282385	0.000007	0.282377
	15-chip 2	11.5	12546	0.00013	0.282394	0.000005	0.282393
Mean observed $^{176}\text{Hf}/^{177}\text{Hf}$ ratio of seven ^c analyses: 0.282393 ± 0.000010 (2s)							
Universität zu Köln	M127-1 (# 6)	55.8	12970	0.0006102	0.282406	0.000004	0.282400
	M127-2 (# 7)	56.8	12956	0.0006223	0.282407	0.000005	0.282401
	M127-3 (# 8)	56.1	12847	0.0006198	0.282403	0.000004	0.282397
	M127-4 (# 9)	54.9	12840	0.0006066	0.282401	0.000004	0.282395
	M127-5 (# 10)	54.7	12631	0.0006142	0.282407	0.000004	0.282401
Mean observed $^{176}\text{Hf}/^{177}\text{Hf}$ ratio of five analyses: 0.282405 ± 0.000005 (2s)							

Results of replicate analyses are quoted but were not considered in the calculation of means.

Note that additional results of Hf isotope determinations, performed by LA-ICP-MS at the Chinese Academy of Sciences, Beijing, are listed in Table S1.

^a M127 data are corrected to analyses of JMC 475.

^b Age-corrected $^{176}\text{Hf}/^{177}\text{Hf}$ ratio (524 Ma).

^c In the calculation of means, results of re-analyses were not considered.

Hafnium isotope determination by LA-ICP-MS

To check the internal homogeneity of the $^{176}\text{Hf}/^{177}\text{Hf}$ ratio, 130 individual LA-ICP-MS analyses were performed using the Neptune MC-ICP-MS system of the Institute of Geology and Geophysics, Chinese Academy of Sciences, Beijing. The JMC 475 standard solution with 200 ng g^{-1} Hf was used for evaluating the reproducibility and accuracy of the instrument prior to laser ablation analyses. During laser ablation determinations of Hf isotopes, the isobaric interference of ^{176}Lu on ^{176}Hf was relatively small compared with the interference of ^{176}Yb on ^{176}Hf , which must be carefully corrected since the contribution of ^{176}Yb to ^{176}Hf can profoundly affect the accuracy of the measured $^{176}\text{Hf}/^{177}\text{Hf}$ ratio (e.g., Fisher *et al.* 2011). Here, the mean $^{173}\text{Yb}/^{171}\text{Yb}$

ratio of all individual spot analyses was used to calculate the fractionation coefficient (β_{Yb}) and then to calculate the contribution of ^{176}Yb to ^{176}Hf using an isotopic ratio of $^{176}\text{Yb}/^{172}\text{Yb} = 0.5887$ (Wu *et al.* 2006). Reference zircon 91500 was used for 'external' correction. During the measurement sessions, the $^{176}\text{Hf}/^{177}\text{Hf}$ value of 91500 was 0.282294 ± 0.000039 (2s, $n = 436$), which was adjusted to 0.282305 (correction of 0.000011), a reference value recommended for 91500 (Wu *et al.* 2006). During data acquisition, analyses of GJ-1 as an unknown yielded a weighted $^{176}\text{Hf}/^{177}\text{Hf}$ ratio of 0.282018 ± 0.000048 (2s, $n = 116$), within error the recommended value (Morel *et al.* 2008). Data are not presented in detail here; they are available online (Table S1; see link given at the end of the paper). Analyses did not yield any significant variations

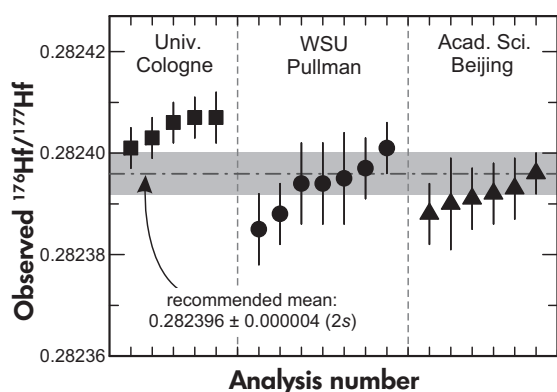


Figure 8. Results of Hf isotope determinations (solution ICP-MS) performed at University of Cologne (five individual analyses), Washington State University, Pullman, WA (seven), and the Chinese Academy of Sciences, Beijing (six). Error bars represent 2s uncertainties.

within and among chips, underlining the homogeneity of zircon M127; the mean $^{176}\text{Hf}/^{177}\text{Hf}$ value of all 130 analyses was 0.282392 ± 0.000031 (2s).

Hafnium isotope determination – discussion

One puzzling observation related to the solution isotope dilution results (Table 4) is the diversity of Lu mass fractions (and, connected with that, of $^{176}\text{Lu}/^{177}\text{Hf}$ ratios). Fairly uniform Lu mass fractions were measured in Köln-Bonn whereas the results of the other two laboratories show a comparably large scatter. These differences could point to sample heterogeneity. Recall, however, that all three laboratories received corresponding fragments recovered from the same areas in the five gemstone slices, so samples may be assumed to represent a nearly identical set. This implies that sample heterogeneity is most likely not the cause of scattered Lu mass fractions, because otherwise similar scatters would be expected to have been found by all three laboratories. Possible other reasons for Lu data variations include difficulties relating spiking subaliquots some time period after dissolution (as done in the RIGL facility and at the IGGCAS). This practice may have resulted in differing behaviour of Hf and Lu during the chemical treatment. For instance, it may be speculated that REE-fluoride complexes might have formed that prevented the spike and sample from equilibrating completely with respect to Lu. We therefore cannot be sure the variations in $^{176}\text{Lu}/^{177}\text{Hf}$ observed by the RIGL and IGGCAS laboratories are real. Rather we assess the Köln-Bonn results as reliable, which suggest the true $^{176}\text{Lu}/^{177}\text{Hf}$ is homogeneous. Thus, we suggest the Köln-Bonn result of $^{176}\text{Lu}/^{177}\text{Hf}$

$= 0.0006146 \pm 0.0000130$ (2s) be used as a ‘working value’ in Hf-Lu studies. It is, however, clear that the possibility of interlaboratory variations needs to be resolved in future measurement campaigns.

Oxygen isotope determination by laser fluorination

Sixteen fragments of zircon M127 (masses in the range 1.83–3.98 mg) were analysed for oxygen isotope ratios at the University of Wisconsin, Madison. Analyses were performed in four separate sessions. The routine procedure at UW is to treat zircons in cold HF for 8 hr before laser fluorination and analysis for oxygen isotope ratios. This procedure removed non-zircon impurities and also dissolved intracrystalline domains that were severely radiation damaged and thus susceptible to postcrystallisation alteration of $\delta^{18}\text{O}$ (Valley *et al.* 2005, 2015); it has been shown not to affect $\delta^{18}\text{O}$ of undamaged zircon (Valley 2003). Two chips that were HF treated for the 10 December 2015, session lost 14% *m/m*, which is more than expected for such clean fragments. The fragments were then pretreated at room temperature in a BrF_5 atmosphere for 12 hr, and each was heated in the presence of fresh BrF_5 , using an infrared laser ($\lambda = 10.6 \mu\text{m}$). The evolved O_2 gas was cryogenically purified, converted to CO_2 and analysed by dual-inlet gas source mass spectrometer as described by Valley *et al.* (1995). Garnet reference material UWG-2 (Valley *et al.* 1995) was analysed four to six times in each analysis session of M127. The $\delta^{18}\text{O}$ values obtained for M127 were normalised to the recommended value of 5.80‰ VSMOW (Vienna Standard Mean Ocean Water) for UWG-2 (Valley *et al.* 1995). Nine analyses of untreated fragments yielded a value of $\delta^{18}\text{O} = 8.26 \pm 0.06\text{‰}$ VSMOW for zircon M127 (Table 4), whereas seven analyses of HF-treated fragments yielded a value of $\delta^{18}\text{O} = 8.49 \pm 0.05\text{‰}$ VSMOW (2s; unweighted means). These data are systematically higher for the HF-treated zircon grains by an average of 0.23‰.

The difference obtained by laser fluorination analysis of M127 between untreated and HF-treated zircon is small and comparable to the measurement precision obtained by *in situ* SIMS analysis. We interpret the HF-treated value as most reliably reflecting the original composition of the M127 zircon. If the HF treatment has selectively removed zircon domains that are slightly higher in $\delta^{18}\text{O}$, then the untreated value for $\delta^{18}\text{O}$ best represents the bulk composition of the M127 crystal. Any higher $\delta^{18}\text{O}$ domains will be included in a SIMS analysis and if present, the homogeneity of SIMS analyses suggests that higher $\delta^{18}\text{O}$ domains are submicrometre and randomly distributed. Thus, the untreated value $\delta^{18}\text{O} = 8.26 \pm 0.06\text{‰}$ VSMOW (2s) is recommended for

Table 4.
Oxygen isotope determinations by laser fluorination (University of Wisconsin at Madison)

Analysis No.	Sample/ reference name	Material analysed	Mass (mg)	$\delta^{18}\text{O}$	
				Raw	(‰ VSMOW) ^a
Measurement session on 22 January 2014					
5	UWG-2	Garnet reference	2.00	5.86	
6	UWG-2	Garnet reference	2.09	5.86	
8	UWG-2	Garnet reference	3.11	5.76	
9	UWG-2	Garnet reference	2.81	5.83	
10	M127	Zircon (HF treated)	3.00	8.50	8.48
11	M127	Zircon (HF treated)	2.40	8.53	8.51
12	M127	Zircon (HF treated)	2.52	8.47	8.45
13	M127	Zircon (HF treated)	3.16	8.54	8.52
14	M127	Zircon (HF treated)	3.16	8.49	8.47
				M127 average: 8.49 ± 0.06 (2s)	
15	UWG-2	Garnet reference	2.74	5.83	
16	UWG-2	Garnet reference	2.12	5.77	
Measurement session on 7 May 2014					
1	UWG-2	Garnet reference	2.92	5.98	
2	UWG-2	Garnet reference	2.26	6.09	
3	UWG-2	Garnet reference	2.37	6.02	
4	UWG-2	Garnet reference	1.86	5.99	
5	UWG-2	Garnet reference	2.90	5.96	
26	M127	Zircon	3.49	8.54	8.32
27	M127	Zircon	2.54	8.47	8.25
28	M127	Zircon	3.98	8.44	8.22
				M127 average: 8.26 ± 0.10 (2s)	
Measurement session on 1 December 2015					
2	UWG-2	Garnet reference	2.90	5.80	
3	UWG-2	Garnet reference	2.37	5.77	
4	UWG-2	Garnet reference	2.74	5.78	
5	UWG-2	Garnet reference	2.14	5.85	
6	UWG-2	Garnet reference	1.72	5.79	
7	M127	Zircon	2.62	8.20	8.24
8	M127	Zircon	2.42	8.24	8.28
9	M127	Zircon	2.60	8.19	8.23
10	M127	Zircon	2.45	8.22	8.26
11	M127	Zircon	2.47	8.25	8.29
				M127 average: 8.26 ± 0.05 (2s)	
12	UWG-2	Garnet reference	2.94	5.65	
13	UWG-2	Garnet reference	2.00	5.74	
14	UWG-2	Garnet reference	2.60	5.73	
15	UWG-2	Garnet reference	2.31	5.76	
Measurement session on 10 December 2015					
2	UWG-2	Garnet reference	2.76	5.80	
3	UWG-2	Garnet reference	2.22	5.76	
4	UWG-2	Garnet reference	1.75	5.73	
5	UWG-2	Garnet reference	1.51	5.76	
6	M127	Zircon (HF treated)	1.97	8.44	8.48
7	M127	Zircon	2.09	8.21	8.25
8	M127	Zircon (HF treated)	1.83	8.45	8.49

Summary:

Zircon M127 (HF treated; seven individual analyses): Average $\delta^{18}\text{O} = 8.49 \pm 0.05$ (2s)

Zircon M127 (non-HF treated; nine individual analyses): Average $\delta^{18}\text{O} = 8.26 \pm 0.06$ (2s)

Note that additional results of O isotope determinations, performed by SIMS at the Chinese Academy of Sciences, Beijing, and the Helmholtz-Zentrum Potsdam (GFZ), are listed in Table S2.

^a M127 data are corrected to the respective UWG-2 reference analyses.

calibration of SIMS analysis with the caveat that there are currently no estimates for the effect of radiation damage on the instrument bias (or instrumental mass fractionation). Although it is usually recommended to use a zircon with less radiation damage for determination of oxygen isotope ratios, such as KIM-5 (Valley 2003), M127 might be a better reference for samples with comparable amounts of damage.

Oxygen isotope determination by SIMS

To check the homogeneity of the oxygen isotope ratio, SIMS analyses were performed at Institute of Geology and Geophysics, Chinese Academy of Sciences, Beijing, and at the Helmholtz-Zentrum Potsdam (GFZ). In Beijing, a total of thirty point analyses placed in six chips originating from five slices of the original stone were performed using a Cameca IMS 1280. The primary Cs^+ beam was accelerated at 10 kV, with a current of 1.2 nA. The spot size was about 20 μm in diameter (10 μm beam diameter plus 10 μm raster). Low-energy electron flooding was used to compensate for sample charging during analysis. Secondary ions were extracted with a -10 kV potential. Oxygen isotopes were measured in multicollection mode with two off-axis Faraday cups. Each analysis consisted of twenty cycles per 4 s counting time. The instrumental mass fractionation factor was corrected using the Penglai zircon reference (with $\delta^{18}\text{O} = 5.3\text{‰}$ VSMOW; see Li *et al.* 2010). Measurement repeatability was better than 0.4‰ (2s) for $\delta^{18}\text{O}$. Calibrated against the Penglai reference, the data set yielded a mean of $\delta^{18}\text{O} = 8.34 \pm 0.34\text{‰}$ VSMOW (2s).

The Potsdam Cameca IMS 1280-HR performed a total of forty-one point analyses on a total of five chips. These five chips were recovered from the five main slices of the original gemstone (see Figure 1b; one chip per slice). These analyses employed a ~ 2.5 nA, mass filtered $^{133}\text{Cs}^+$ beam with a Gaussian density distribution, which was focussed to a ~ 5 μm diameter on the polished sample surface. The total impact energy of the Cs^+ ions was 20 keV. Each analysis was preceded by 20 $\mu\text{m} \times 20$ μm rastered presputter for 60 s. The total pressure in the sample chamber was 1×10^{-7} Pa at the time of analysis. Charge compensation was achieved with low-energy, normal-incidence electron flooding using a current of ~ 1 μA . All analyses were conducted in duplicate in sequence with an offset between the two analytical locations of 50 μm , to assess the short-term stability of our technique. To suppress within-run drift in the isotope ratio, a 10 $\mu\text{m} \times 10$ μm raster was employed during data collection, thus assuring a crater geometry with a flat bottom. Secondary ions were accelerated by a -10 kV potential applied to the sample holder. The mass spectrometer was operated in static multicollection mode, with the

$^{16}\text{O}^-$ being collected in the L2' Faraday cup and the $^{18}\text{O}^-$ signal being collected in the H2' Faraday cup; the amplifier system employed thermally stabilised $10^{10} \Omega$ and $10^{11} \Omega$ amplifiers, respectively. The mass resolution of the instrument was determined to be $M/\Delta M \approx 1670$ on the ^{16}O mass station and $M/\Delta M \approx 1970$ on the ^{18}O mass station. This is effectively full transmission for the tool and fully suffices to eliminate both the $^{16}\text{O}^1\text{H}_2$ and the $^{16}\text{O}^2\text{H}$ isobaric interferences from the ^{18}O mass station. A single analysis consisted of twenty integrations of 4 s each. Using white-light profilometry, we determined that the test portion mass for our analyses was equivalent to ca. 150 picograms. Data for M127 were corrected for instrumental mass fractionation using the 91500 reference (with $\delta^{18}\text{O} = 9.86\text{‰}$ VSMOW; see Wiedenbeck *et al.* 2004). Analysis on M127 yielded a mean of $\delta^{18}\text{O} = 7.96 \pm 0.20\text{‰}$ VSMOW (2s) for forty-one determinations on the five fragments, meaning this data set is consistent with being a homogeneous population.

Data are available online (see supporting information Table S2). No systematic variations or 'outliers' were found among the thirty analyses in the Beijing laboratory. Among the forty-one analyses in Potsdam, two measurements in a single area gave results 0.25‰ lighter than the remainder of the population, and suspiciously, these were the first data acquired during our measurement series. Discarding these two, seemingly discrepant, values yielded a measurement repeatability of $\pm 0.16\text{‰}$ (2s) on $n = 39$ determinations, indicating that M127 is at least as homogeneous as the 91500 zircon, which we presume to be homogeneous in its $\delta^{18}\text{O}$ content. We therefore conclude that M127 is well suited for use as a reference material in SIMS studies that correlate U–Pb age and $\delta^{18}\text{O}$ of unknown zircon samples (see Cavosie *et al.* 2005, Valley *et al.* 2005).

Oxygen isotope determination – discussion

Unlike the homogeneous Sri Lanka zircon references CZ3 (Cavosie *et al.* 2011) and M257 (Nasdala *et al.* 2008), the $\delta^{18}\text{O}$ value determined for zircon M127 is not remarkably high and hence does not fall outside the range typical of igneous zircon (Figure 9). Unlike CZ3 and M257, the oxygen isotope ratio of M127 does not provide a clear indication of the formation environment (whereas the particularly high $\delta^{18}\text{O}$ values of some Sri Lanka zircon samples are presumed to indicate formation in a marble or Ca silicate metamorphic rock; Cavosie *et al.* 2011). We can therefore merely speculate that the remarkable homogeneity (i.e., absence of all signs of 'igneous' growth zoning) of zircon M127 might be explained by (a) metamorphic formation that, however, did not result in a very high $\delta^{18}\text{O}$ value or (b) igneous formation that must

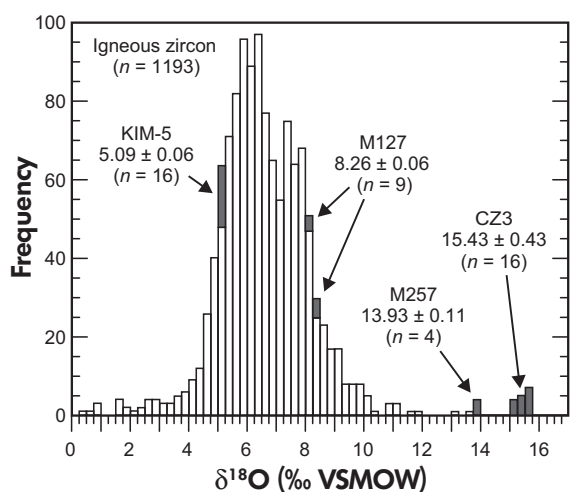


Figure 9. Plot of $\delta^{18}\text{O}$ data for zircon M127 (laser fluorination; University of Wisconsin, Madison) and data for references KIM-5 (Valley 2003), M257 (Nasdala *et al.* 2008) and CZ3 (Cavosie *et al.* 2011) in comparison with those for igneous zircon from localities world-wide (Valley *et al.* 2005).

have resulted in the formation in particularly thick growth zones. As zircon M127 was derived from a gem gravel, with the original host rock being unknown, the formation environment remains uncertain.

Lithium isotope determination by SIMS

Lithium isotope determinations were performed using the Cameca IMS-1280 HR at the Institute of Geology and Geophysics, Chinese Academy of Sciences, Beijing. A detailed description of the procedure followed can be found in Li *et al.* (2011), and therefore, only a brief description is given here. The primary O^- ion beam was accelerated at -13 kV, with a beam current of 28 nA. The

beam was focussed to an elliptical spot ca. 20–30 μm in size. Positive secondary ions were extracted with a 10 kV potential. A single ion-counting electron multiplier (EM) was used as the detection device. The mass resolution was 1300 (at 10% peak height). Each measurement consisted of eighty cycles, with a total measurement time of 20 min. The M257 zircon reference ($\text{Li} = 0.86 \mu\text{g g}^{-1}$ and $\delta^7\text{Li} = 2.1 \pm 1.0\text{‰}$; see Li *et al.* 2011) was used as calibrant material.

A total of fifty-five analyses were performed on six fragments of M127 that were embedded in a polished epoxy sample mount. The mean Li mass fraction of zircon M127 is $1.0 \pm 0.1 \mu\text{g g}^{-1}$ (2s), and the mean $\delta^7\text{Li}$ value was determined at $-0.6 \pm 0.9\text{‰}$ (2s). This can initially be used as a working value for M127, although there is an urgent need for further characterisation of this system using other, independent analytical methods (i.e., solution ICP-MS). In view of the low $\delta^7\text{Li}$ variability observed in this study, M127 may be a useful reference material in SIMS studies that use Li as a petrogenetic tracer (Ushikubo *et al.* 2008, Li *et al.* 2011, Bouvier *et al.* 2012).

(U–Th)/He analysis

The retention of the radiogenic ^4He was evaluated by (U–Th)/He analyses at the University of Arizona, Tucson. Our experimental details are described elsewhere (Nasdala *et al.* 2004, Reiners 2005), and our results are presented in Table 5. Analyses on chips M127zA and M127zB were performed in 2006, in the course of the characterisation of zircon M257; the other chips were analysed in 2015. All five analyses yielded a weighted mean He age of $426 \pm 7 \text{ Ma}$ (2s) for zircon M127. This value is well within the range of typical helium ages for unheated zircon samples from Sri Lanka (Hurley 1954, Nasdala *et al.* 2004). It also confirms that zircon M127 has never been subjected to heat treatment, as this would have caused near total loss of radiogenic helium (Reiners 2005).

Table 5.
(U+Th)/He age of M127 (University of Arizona at Tucson)

Sample name	^4He (pmol)	U (ng)	Th (ng)	Age (Ma)
M127zA	11.6 ± 0.2	4.41 ± 0.16	2.04 ± 0.06	425 ± 17
M127zB	24.2 ± 0.6	9.24 ± 0.34	4.26 ± 0.14	423 ± 18
15B346	0.809 ± 0.010	0.303 ± 0.008	0.133 ± 0.004	432 ± 12
15B347	2.05 ± 0.06	0.772 ± 0.024	0.341 ± 0.010	428 ± 17
15B348	0.227 ± 0.006	0.088 ± 0.002	0.041 ± 0.002	417 ± 18
Weighted mean age of five analyses: $426 \pm 7 \text{ Ma}$ (2s)				

All analytical uncertainties are 2s.

Conclusions

Zircon M127 is a suitable reference material for the SIMS U–Pb analysis of unknown zircon samples, especially in studies that subject the same sample mounts to the additional analysis of oxygen (SIMS), lithium (SIMS) or hafnium isotopes (LA-ICP-MS). Zircon M127 is homogeneous in terms of chemical and isotopic composition and has a remarkably concordant U–Pb isotopic system. Therefore, M127 is suitable for calibration, quality control and method validation purposes for analytical techniques working at the low- to subnanogram sampling scale, and its broad acceptance by the SIMS community would greatly improve the metrological traceability between facilities. A particularly advantageous property of M127 is the fairly high uranium mass fraction of $\sim 923 \mu\text{g g}^{-1}$ (and correspondingly high levels of radiogenic Pb), which will result in exceptionally high count rates and good counting statistics for SIMS analyses.

The material will in future be used and distributed by the Beijing SHRIMP Centre, Institute of Geology, Chinese Academy of Geological Sciences (contact: liudunyi@bjshrimp.cn). Zircon M127 is reserved as SIMS reference. In particular, it will not be provided for only U–Pb geochronology in LA-ICP-MS laboratories. Despite this decision, it will of course be possible, and worthwhile, to subject repolished SIMS mounts containing M127 to subsequent analyses by means of LA-ICP-MS, including Hf isotope or LASS (laser ablation split stream method for combined U–Pb and Hf analyses; Fisher *et al.* 2014). This decision was made to reduce the consumption of zircon M127 to a minimum and ensure that the material will be available for SIMS work for several more years.

Acknowledgements

This article is dedicated to Jan Košler (University of Bergen, Norway), who passed away in 2014 at the age of 49. Jan was involved in the initial characterisation of zircon M127. Gem zircon M127 was made available by the Institut für Edelsteinforschung Idar-Oberstein, Germany. Thanks are due to A. Wagner and U. Dittmann for sample preparation. We are indebted to U. Chowdhury, F. Couffignal, G. Giester, A. Kidane, J. Košler (deceased), K. Scheidl and J. Sláma for experimental assistance and to O. Appelt and U. Schaltegger for data and helpful discussions. Synthetic zircon, hafnon, thorite and uranium oxide crystals were provided as EPMA calibrants by J.M. Hanchar. The Penglai zircon was provided by X.-H. Li. Constructive comments by two anonymous reviewers and editor T. Meisel helped to improve the manuscript.

Financial support by the Faculty of Geosciences, Geography and Astronomy, University of Vienna, and the Beijing SHRIMP Centre, Chinese Academy of Geological Sciences, is gratefully acknowledged. Partial funding of this research was provided by the European Commission through contract no. MEXC-CT-2005-024878 to LN, by the FWF Austrian Science Fund through grants P20028-N10 and P24448-N19 to LN. and by the U.S. National Science Foundation, EAR 1524336 to J.W.V.

References

- Andersen C.A. and Hinthorne J.R. (1972)**
Ion microprobe mass analyzer. *Science*, **175**, 853–860.
- Armstrong J.T. (1991)**
Quantitative elemental analysis of individual microparticles with electron beam instruments. In: Heinrich K.F.J. and Newbury D.E. (eds), *Electron probe quantitation*. Plenum Press (New York, London), 261–315.
- Armstrong J.T. (1995)**
CITZAF: A package of correction programs for the quantitative electron microbeam X-ray analysis of thick polished materials, thin films, and particles. *Microbeam Analysis*, **4**, 177–200.
- Bouvier A.S., Ushikubo T., Kita N.T., Cavosie A.J., Kozdon R. and Valley J.W. (2012)**
Li isotopes and trace elements as a petrogenetic tracer in zircon: Insights from Archean TTGs and sanukitoids. *Contributions to Mineralogy and Petrology*, **163**, 745–768.
- Cavosie A.J., Valley J.W., Wilde S.A. and E.I.M.F. (2005)**
Magmatic $\delta^{18}\text{O}$ in 4400–3900 Ma detrital zircons: A record of the alteration and recycling of crust in the early Archean. *Earth and Planetary Science Letters*, **235**, 663–681.
- Cavosie A.J., Valley J.W., Kita N.T., Spicuzza M.J., Ushikubo T. and Wilde S.A. (2011)**
The origin of high $\delta^{18}\text{O}$ zircons: Marbles, megacrysts, and metamorphism. *Contributions to Mineralogy and Petrology*, **162**, 961–974.
- Compston W., Williams I.S. and Meyer C. (1984)**
U–Pb geochronology of zircon from lunar breccia 73217 using a sensitive high mass-resolution ion microprobe. *Journal of Geophysical Research*, **89**, 525–534.
- Condon D.J., McLean N.M., Schoene B., Bowring S.A., Parrish R.R. and Noble S. (2008)**
Synthetic U–Pb ‘standard’ solutions for ID-TIMS geochronology. *Geochimica et Cosmochimica Acta*, **72**, A175.
- Corfu F. (2004)**
U–Pb age, setting, and tectonic significance of the anorthosite-mangerite-chamockite-granite-suite, Lofoten-Vesterålen, Norway. *Journal of Petrology*, **45**, 1799–1819.

references

Corfu F., Hanchar J.M., Hoskin P.W.O. and Kinny P. (2003)

Atlas of zircon textures. In: Hanchar J.M. and Hoskin P.W.O. (eds), *Zircon. Reviews in Mineralogy and Geochemistry*, 53, Mineralogical Society of America (Chantilly, VA, USA), 469–500.

Dijkman F.G. and van der Maas J.H. (1976)

Dependence of band shape and depolarization ratio on slit width. *Applied Spectroscopy*, 30, 545–546.

Fisher C.M., Hanchar J.M., Samson S.D., Dhuime B., Blichert-Toft J., Vervoort J.D. and Lam R. (2011)

Synthetic zircon doped with hafnium and rare earth elements: A reference material for *in situ* hafnium isotope analysis. *Chemical Geology*, 286, 32–47.

Fisher C.M., Vervoort J.D. and DuFrane S.A. (2014)

Accurate Hf isotope determinations of complex zircons using the “laser ablation split stream” method. *Geochemistry, Geophysics, Geosystems*, 15, 121–139.

Gaft M., Panczer G., Reinfeld R. and Shinno I. (2000)

Laser-induced luminescence of rare-earth elements in natural zircon. *Journal of Alloys and Compounds*, 300–301, 267–274.

Geisler T., Rashwan A.A., Rahn M.K.W., Poller U., Zwingmann H., Pidgeon R.T., Schleicher H. and Tomaschek F. (2003)

Low-temperature hydrothermal alteration of natural metamict zircon from the Eastern Desert, Egypt. *Mineralogical Magazine*, 67, 485–508.

Goode J.W. and Vervoort J.D. (2006)

Origin of Mesoproterozoic A-type granites in Laurentia: Hf isotope evidence. *Earth and Planetary Science Letters*, 243, 711–731.

Guenther W.R., Reiners P.W., Ketchum R.A., Nasdala L. and Giester G. (2013)

Helium diffusion in natural zircon: Radiation damage, anisotropy, and the interpretation of zircon (U-Th)/He thermochronology. *American Journal of Science*, 313, 145–198.

Holland H.D. (1954)

Radiation damage and its use in age determination. In: Faul H. (ed.), *Nuclear geology*. Wiley (New York), 175–179.

Holland H.D. and Gottfried D. (1955)

The effect of nuclear radiation on the structure of zircon. *Acta Crystallographica*, 8, 291–300.

Hoskin P.W.O. and Schaltegger U. (2003)

The composition of zircon and igneous and metamorphic petrogenesis. In: Hanchar J.M. and Hoskin P.W.O. (eds), *Zircon. Reviews in Mineralogy and Geochemistry*, 53, 27–62.

Hurley P.M. (1954)

The helium age method and the distribution and migration of helium in rocks. In: Faul H. (ed.), *Nuclear geology*. Wiley (New York), 301–329.

Jaffey A.H., Flynn K.F., Glendenin L.E., Bentley W.C. and Essling A.M. (1971)

Precision measurement of half-lives and specific activities of ^{235}U and ^{238}U . *Physical Review C*, 4, 1889–1906.

Kennedy A.K. (2000)

The search for new zircon standards for SIMS. In: Woodhead J.D., Hergt J.M. and Noble W.P. (eds), *Beyond 2000: New frontiers in isotope geoscience (incorporating ACOG 4)*, Lorne, Australia. Abstracts and Proceedings. Eastern Press (Mulgrave, VIC, Australia), 109–111.

Krogh T.E. (1973)

A low contamination method for the hydrothermal decomposition of zircon and extraction of U and Pb for isotopic age determinations. *Geochimica et Cosmochimica Acta*, 37, 485–494.

Kröner A., Kehelpannala K.V.W. and Kriegsman L.M. (1994)

Origin of compositional layering and mechanism of crustal thickening in the high-grade gneiss terrain of Sri Lanka. *Precambrian Research*, 66, 21–37.

Lenz C. and Nasdala L. (2015)

A photoluminescence study of REE $^{3+}$ emissions in radiation-damaged zircon. *American Mineralogist*, 100, 1123–1133.

Lenz C., Nasdala L., Talla D., Hauzenberger C., Seitz R. and Kolitsch U. (2015)

Laser-induced REE $^{3+}$ photoluminescence of selected accessory minerals – An “advantageous artefact” in Raman spectroscopy. *Chemical Geology*, 415, 1–16.

Li X.-H., Long W.-G., Li Q.-L., Liu Y., Zheng Y.-F., Yang Y.-H., Chamberlain K.R., Wan D.-F., Guo C.-H., Wang X.-C. and Tao H. (2010)

Penglai zircon megacrysts: A potential new working reference material for microbeam determination of Hf-O isotopes and U-Pb age. *Geostandards and Geoanalytical Research*, 34, 117–134.

Li X.-H., Li Q.-L., Liu Y. and Tang G.Q. (2011)

Further characterization of M257 zircon standard: A working reference for SIMS analysis of Li isotopes. *Journal of Analytical Atomic Spectrometry*, 26, 352–358.

Ludwig K.R. (2003)

User’s manual for Isoplot 3.00: A geochronological toolkit for Microsoft Excel, 4. Berkeley Geochronology Center Special Publication (Berkeley), 71 pp.

Mattinson J.M. (2010)

Analysis of the relative decay constants of ^{235}U and ^{238}U by multi-step CA-TIMS measurements of closed-system natural zircon samples. *Chemical Geology*, 275, 186–198.

Mattinson J.M., Nasdala L., Lengauer C. and Wirth R. (2007)

Inside CA-TIMS zircon analysis: The interplay among natural radiation damage, annealing, solubility, and U-Pb isotopic systematics. *EOS, Transactions, American Geophysical Union*, 88, 52, Supplement, abstract V31G-06.

references

- McLaren A.C., FitzGerald J.D. and Williams I.S. (1994)**
The microstructure of zircon and its influence on the age determination from Pb/U isotopic ratios measured by ion microprobe. *Geochimica et Cosmochimica Acta*, 58, 993–1005.
- Morel M.L.A., Nebel O., Nebel-Jacobsen Y., Miller J.S. and Vroon P.Z. (2008)**
Hafnium isotope characterization of the GJ-1 zircon reference material by solution and laser-ablation MC-ICP-MS. *Chemical Geology*, 255, 213–235.
- Munasinghe T. and Dissanayake C.B. (1981)**
The origin of gemstones in Sri Lanka. *Economic Geology*, 76, 1216–1225.
- Münker C., Weyer S., Scherer E.E. and Mezger K. (2001)**
Separation of high field-strength elements (Nb, Ta, Zr, Hf) and Lu from rock samples for MC-ICP-MS measurements. *Geochemistry, Geophysics, Geosystems*, 2, 1064. doi:10.1029/2001GC000183.
- Murakami T., Chakoumakos B.C., Ewing R.C., Lumpkin G.R. and Weber W.J. (1991)**
Alpha-decay event damage in zircon. *American Mineralogist*, 76, 1510–1532.
- Nasdala L., Imer G. and Wolf D. (1995)**
The degree of metamictization in zircons: A Raman spectroscopic study. *European Journal of Mineralogy*, 7, 471–478.
- Nasdala L., Wenzel M., Vavra G., Imer G., Wenzel T. and Kober B. (2001)**
Metamictisation of natural zircon: Accumulation versus thermal annealing of radioactivity-induced damage. *Contributions to Mineralogy and Petrology*, 141, 125–144.
- Nasdala L., Lengauer C.L., Hanchar J.M., Kronz A., Wirth R., Blanc P., Kennedy A.K. and Seydoux-Guillaume A.-M. (2002)**
Annealing radiation damage and the recovery of cathodoluminescence. *Chemical Geology*, 191, 121–140.
- Nasdala L., Reiners P.W., Garver J.J., Kennedy A.K., Stern R.A., Balan E. and Wirth R. (2004)**
Incomplete retention of radiation damage in zircon from Sri Lanka. *American Mineralogist*, 89, 219–231.
- Nasdala L., Hofmeister W., Norberg N., Mattinson J.M., Corfu F., Dörr W., Kamo S.L., Kennedy A.K., Kronz A., Reiners P.W., Frei D., Košler J., Wan Y., Götz J., Häger T., Kröner A. and Valley J.W. (2008)**
Zircon M257 – A homogeneous natural reference material for the ion microprobe U-Pb analysis of zircon. *Geostandards and Geoanalytical Research*, 32, 247–265.
- Nasdala L., Hanchar J.M., Rhede D., Kennedy A.K. and Váci T. (2010)**
Retention of uranium in complexly altered zircon: An example from Bancroft, Ontario. *Chemical Geology*, 269, 290–300.
- Nebel-Jacobsen Y., Scherer E.E., Münker C. and Mezger K. (2005)**
Separation of U, Pb, Lu and Hf from single zircons for combined U-Pb dating and Hf isotope measurements by TIMS and MC-ICP-MS. *Chemical Geology*, 220, 105–120.
- Norberg N. (2007)**
Characterization of two zircon gemstones in view of their potential suitability as international age determination standards. Diploma thesis, Universität Wien.
- Palenik C.S., Nasdala L. and Ewing R.C. (2003)**
Radiation damage in zircon. *American Mineralogist*, 88, 770–781.
- Patchett P.J. and Tatsumoto M. (1980)**
A routine high-precision method for Lu–Hf isotope geochemistry and chronology. *Contributions to Mineralogy and Petrology*, 75, 263–267.
- Pérez-Soba C., Villaseca C., González del Tánago J. and Nasdala L. (2007)**
The composition of zircon in the peraluminous Hercynian granites of the Spanish Central System batholith. *Canadian Mineralogist*, 45, 509–527.
- Pidgeon R.T. (1997)**
Zirkon in edelsteinqualität: Seine verwendung als standardmaterial in der geologischen zeitbestimmung mit ionensonden. *Zeitschrift der Deutschen Gemmologischen Gesellschaft*, 46, 21–28.
- Reiners P.W. (2005)**
Zircon (U-Th)/He thermochronometry. In: Reiners P.W. and Ehlers T.A. (eds), *Low-temperature thermochronology: Techniques, interpretations, and applications*. *Reviews in Mineralogy and Geochemistry*, 58, 151–179.
- Sahama T.G. (1981)**
Growth structure in Ceylon zircon. *Bulletin de Minéralogie*, 104, 89–94.
- Salje E.K.H., Chrosch J. and Ewing R.C. (1999)**
Is "metamictization" of zircon a phase transition? *American Mineralogist*, 84, 1107–1116.
- Schmitz M.D. and Schoene B. (2007)**
Derivation of isotope ratios, errors, and error correlations for U-Pb geochronology using ^{205}Pb - ^{235}U -(^{233}U)-spiked isotope dilution thermal ionization mass spectrometric data. *Geochemistry, Geophysics, Geosystems*, 8, Q08006. doi:10.1029/2006GC001492.
- Schneider C.A., Rasband W.S. and Eliceiri K.W. (2012)**
NIH Image to ImageJ: 25 years of image analysis. *Nature Methods*, 9, 671–675.
- Schoene B., Crowley J.L., Condon D.J., Schmitz M.D. and Bowring S.A. (2006)**
Reassessing the uranium decay constants for geochronology using ID-TIMS U-Pb data. *Geochimica et Cosmochimica Acta*, 70, 426–445.



references

Smith D.G.W., de St. Jorre L., Reed S.J.B. and Long J.V.P. (1991)

Zonally metamictized and other zircons from Thor Lake, Northwest Territories. *Canadian Mineralogist*, 29, 301–309.

Ushikubo T., Kita N.T., Cavosie A.J., Wilde S.A., Rudnick R.L. and Valley J.W. (2008)

Lithium in Jack Hills zircons: Evidence for extensive weathering of Earth's earliest crust. *Earth and Planetary Science Letters*, 272, 666–676.

Vácz T. (2014)

A new, simple approximation for the deconvolution of instrumental broadening in spectroscopic band profiles. *Applied Spectroscopy*, 68, 1274–1278.

Vácz T., Nasdala L., Wirth R., Mehofer M., Libowitzky E. and Häger T. (2009)

On the breakdown of zircon upon “dry” thermal annealing. *Mineralogy and Petrology*, 97, 129–138.

Valley J.W. (2003)

Oxygen isotopes in zircon. In: Hanchar J.M. and Hoskin P.W.O. (eds), *Zircon. Reviews in Mineralogy and Geochemistry*, 53, 343–385.

Valley J.W., Kitchen N.E., Kohn M.J., Niendorf C.R. and Spicuzza M.J. (1995)

UWG-2 - A garnet standard for oxygen isotope ratios: Strategies for high precision and accuracy with laser heating. *Geochimica et Cosmochimica Acta*, 59, 5223–5231.

Valley J.W., Lackey J.S., Cavosie A.J., Clechenko C.C., Spicuzza M.J., Basei M.A.S., Bindeman I.N., Ferreira V.P., Sial A.N., King E.M., Peck W.H., Sinha A.K. and Wei C.S. (2005)

4.4 billion years of crustal maturation: Oxygen isotope ratios of magmatic zircon. *Contributions to Mineralogy and Petrology*, 150, 561–580.

Valley J.W., Reinhard D.A., Cavosie A.J., Ushikubo T., Lawrence D.F., Larson D.J., Kelly T.F., Snoeyenbos D. and Strickland A. (2015)

Nano- and micro-geochronology in Hadean and Archean zircons by atom-probe tomography and SIMS: New tools for old minerals. *American Mineralogist*, 100, 1355–1377.

Vervoort J.D., Patchett P.J., Soderlund U. and Baker M. (2004)

Isotopic composition of Yb and the determination of Lu concentrations and Lu/Hf by isotope dilution using MC-ICP-MS. *Geochemistry, Geophysics, Geosystems*, 5, Q11002. doi:10.1029/2003GC000582.

Weber W.J. (1990)

Radiation-induced effects and amorphization in zircon. *Journal of Materials Research*, 5, 2687–2697.

Weber W.J. (1993)

Alpha-decay-induced amorphization in complex silicate structures. *Journal of the American Ceramic Society*, 76, 1729–1738.

Wiedenbeck M., Hanchar J.M., Peck W.P., Sylvester P., Valley J., Whitehouse M.J., Kronz A., Morishita Y., Nasdala L., Fiebig J., Franchi I., Girard J.P., Greenwood R.C., Hinton R., Kita N., Mason P.R.D., Norman M., Ogasawara M., Piccoli R., Rhede D., Satoh H., Schulz-Dobrick B., Skär O., Spicuzza M.J., Terada K., Tindle A., Togashi S., Vennemann T., Xie Q. and Zheng Y.F. (2004)
Further characterization of the 91500 zircon crystal. *Geostandards and Geoanalytical Research*, 28, 9–39.

Williams I.S. (1998)

U-Th-Pb geochronology by ion microprobe. In: McKibben M.A., Shanks W.C. III and Ridley W.I. (eds), *Applications of microanalytical techniques to understanding mineralizing processes. Reviews in Economic Geology*, 7, 1–35.

Wirth R. (2004)

Focused Ion Beam (FIB): A novel technology for advanced application of micro- and nanoanalysis in geosciences and applied mineralogy. *European Journal of Mineralogy*, 16, 863–876.

Wu F.Y., Yang Y.H., Xie L.W., Yang J.H. and Xu P. (2006)

Hf isotopic compositions of the standard zircons and baddeleyites used in U-Pb geochronology. *Chemical Geology*, 234, 105–126.

Yang Y.H., Zhang H.F., Chu Z.Y., Xie L.W. and Wu F.Y. (2010)

Combined chemical separation of Lu, Hf, Rb, Sr, Sm and Nd from a single rock digest and precise and accurate isotope determinations of Lu-Hf, Rb-Sr and Sm-Nd isotope systems using multi-collector ICP-MS and TIMS. *International Journal of Mass Spectrometry*, 290, 120–126.

Zhang M., Salje E.K.H., Faman I., Graeme-Barber A., Daniel P., Ewing R.C., Clark A.M. and Lennox H. (2000)

Metamictization of zircon: Raman spectroscopic study. *Journal of Physics: Condensed Matter*, 12, 1915–1925.

Zoysa G. (2014)

The geology and gem deposits of Sri Lanka. *InColor*, 27, 38–41.

Supporting information

The following supporting information may be found in the online version of this article:

Table S1. Results of a total of 130 Hf isotope determinations by LA-ICP-MS (six measurement sessions 2009–2013) at the Chinese Academy of Sciences, Beijing

Table S2. Results of O isotope determinations by SIMS at the Chinese Academy of Sciences, Beijing, and the Helmholtz-Zentrum Potsdam (GFZ)

This material is available as part of the online article from: <http://onlinelibrary.wiley.com/doi/10.1111/ggr.12123> (This link will take you to the article abstract).